



# CERTIFICATE OF ACCREDITATION

## The ANSI National Accreditation Board

Hereby attests that

**Transcat – San Diego**  
**10130 Sorrento Valley Rd, Suites C-D**  
**San Diego, CA 92121**

Fulfills the requirements of

**ISO/IEC 17025:2017**

and national standard

**ANSI/NCSL Z540-1-1994 (R2002)**

In the field of

**CALIBRATION**

This certificate is valid only when accompanied by a current scope of accreditation document.  
The current scope of accreditation can be verified at [www.anab.org](http://www.anab.org).

Jason Stine, Vice President

Expiry Date: 01 September 2026  
Certificate Number: L2214



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.  
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory  
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

## SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

AND

ANSI/NCSL Z540-1-1994 (R2002)

**Transcat – San Diego**

10130 Sorrento Valley Rd, Suites C-D

San Diego, CA 92121

Javier Estrada 858-621-2630

### CALIBRATION

ISO/IEC 17025 Accreditation Granted: **01 September 2024**

Certificate Number: **L2214**

Certificate Expiry Date: **01 September 2026**

#### Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Current – Source <sup>2</sup>	Up to 220 $\mu$ A (0.22 to 2.2) mA (2.2 to 22) mA (22 to 220) mA (0.22 to 2.2) A	45 $\mu$ A/A + 6.9 nA 39 $\mu$ A/A + 8.1 nA 39 $\mu$ A/A + 46 nA 58 $\mu$ A/A + 0.7 $\mu$ A 0.24 mA/A + 12 $\mu$ A	Comparison to Fluke 5720A Multiproduct Calibrator
DC Voltage – Source <sup>2</sup>	Up to 220 mV (0.22 to 2.2) V (2.2 to 11) V (11 to 22) V (22 to 220) V (220 to 1 000) V	9.1 $\mu$ V/V + 0.4 $\mu$ V 5.7 $\mu$ V/V + 0.7 $\mu$ V 4.4 $\mu$ V/V + 2.5 $\mu$ V 4 $\mu$ V/V + 4 $\mu$ V 6.3 $\mu$ V/V + 40 $\mu$ V 7.6 $\mu$ V + 0.4 mV	Comparison to Fluke 5720A Multiproduct Calibrator
AC Current – Source <sup>2</sup>	Up to 220 $\mu$ A (10 to 20) Hz (20 to 40) Hz 40 Hz to 1 kHz (1 to 5) kHz (5 to 10) kHz	0.032 % of reading + 16 nA 0.019 % of reading + 10 nA 0.014 % of reading + 8 nA 0.026 % of reading + 10 nA 0.11 % of reading + 65 nA	Comparison to Fluke 5720A Multiproduct Calibrator

**Electrical – DC/Low Frequency**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Current – Source <sup>2</sup>	(0.22 to 2.2) mA		Comparison to Fluke 5720A Multiproduct Calibrator
	(10 to 20) Hz	0.031 % of reading + 40 nA	
	(20 to 40) Hz	0.019 % of reading + 35 nA	
	40 Hz to 1 kHz	0.014 % of reading + 35 nA	
	(1 to 5) kHz	0.026 % of reading + 0.11 µA	
	(5 to 10) kHz	0.11 % of reading + 0.65 µA	
	(2.2 to 22) mA		
	(10 to 20) Hz	0.033 % of reading + 0.4 µA	
	(20 to 40) Hz	0.02 % of reading + 0.35 µA	
	40 Hz to 1 kHz	0.015 % of reading + 0.35 µA	
	(1 to 5) kHz	0.022 % of reading + 0.55 µA	
	(5 to 10) kHz	0.11 % of reading + 5 µA	
	(22 to 220) mA		
	(10 to 20) Hz	0.033 % of reading + 4 µA	
	(20 to 40) Hz	0.018 % of reading + 3.5 µA	
AC Voltage – Source <sup>2</sup>	40 Hz to 1 kHz	0.014 % of reading + 2.5 µA	Comparison to Fluke 5720A Multiproduct Calibrator
	(1 to 5) kHz	0.021 % of reading + 3.5 µA	
	(5 to 10) kHz	0.11 % of reading + 10 µA	
	(0.22 to 2.2) A		
	20 Hz to 1 kHz	0.047 % of reading + 0.17 mA	
	(1 to 5) kHz	0.095 % of reading + 0.38 mA	
	(5 to 10) kHz	0.36 % of reading + 0.16 mA	
	Up to 2.2 mV		
	(10 to 20) Hz	0.16 % of reading + 4 µV	
	(20 to 40) Hz	0.1 % of reading + 4 µV	
	40 Hz to 20 kHz	0.077 % of reading + 4 µV	
	(20 to 50) kHz	0.12 % of reading + 4 µV	
	(50 to 100) kHz	0.17 % of reading + 5 µV	
	(100 to 300) kHz	0.33 % of reading + 10 µV	
	(300 to 500) kHz	0.47 % of reading + 20 µV	
	500 kHz to 1 MHz	0.58 % of reading + 20 µV	
	(2.2 to 22) mV		
	(10 to 20) Hz	0.044 % of reading + 4 µV	
	(20 to 40) Hz	0.031 % of reading + 4 µV	
	40 Hz to 20 kHz	0.015 % of reading + 4 µV	
	(20 to 50) kHz	0.031 % of reading + 4 µV	
	(50 to 100) kHz	0.059 % of reading + 5 µV	
	(100 to 300) kHz	0.12 % of reading + 10 µV	
	(300 to 500) kHz	0.16 % of reading + 20 µV	
	500 kHz to 1 MHz	0.3 % of reading + 20 µV	

**Electrical – DC/Low Frequency**

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
AC Voltage – Source <sup>2</sup>	(22 to 220) mV		Comparison to Fluke 5720A Multiproduct Calibrator
	(10 to 20) Hz	0.028 % of reading + 12 $\mu$ V	
	(20 to 40) Hz	0.011 % of reading + 7 $\mu$ V	
	40 Hz to 20 kHz	0.009 % of reading + 7 $\mu$ V	
	(20 to 50) kHz	0.021 % of reading + 7 $\mu$ V	
	(50 to 100) kHz	0.047 % of reading + 17 $\mu$ V	
	(100 to 300) kHz	0.092 % of reading + 20 $\mu$ V	
	(300 to 500) kHz	0.14 % of reading + 25 $\mu$ V	
	500 kHz to 1 MHz	0.28 % of reading + 45 $\mu$ V	
	(0.22 to 2.2) V		
	(10 to 20) Hz	0.028 % of reading + 40 $\mu$ V	
	(20 to 40) Hz	0.01 % of reading + 15 $\mu$ V	
	40 Hz to 20 kHz	0.005 % of reading + 8 $\mu$ V	
	(20 to 50) kHz	0.008 % of reading + 10 $\mu$ V	
	(50 to 100) kHz	0.012 % of reading + 30 $\mu$ V	
	(100 to 300) kHz	0.043 % of reading + 80 $\mu$ V	
	(300 to 500) kHz	0.1 % of reading + 0.2 mV	
	500 kHz to 1 MHz	0.18 % of reading + 0.3 mV	
	(2.2 to 22) V		
	(10 to 20) Hz	0.028 % of reading + 0.4 mV	
	(20 to 40) Hz	0.01 % of reading + 0.15 mV	
	40 Hz to 20 kHz	0.005 % of reading + 50 $\mu$ V	
	(20 to 50) kHz	0.008 % of reading + 0.1 mV	
	(50 to 100) kHz	0.011 % of reading + 0.2 mV	
	(100 to 300) kHz	0.03 % of reading + 0.6 mV	
	(300 to 500) kHz	0.1 % of reading + 2 mV	
	500 kHz to 1 MHz	0.17 % of reading + 3.2 mV	
	(22 to 220) V		
	(10 to 20) Hz	0.028 % of reading + 4 mV	
	(20 to 40) Hz	0.01 % of reading + 1.5 mV	
	40 Hz to 20 kHz	0.006 % of reading + 0.6 mV	
	(20 to 50) kHz	0.009 % of reading + 1 mV	
	(50 to 100) kHz	0.016 % of reading + 2.5 mV	
	(100 to 300) kHz	0.09 % of reading + 16 mV	
	(220 to 750) V		
	(30 to 50) kHz	0.061 % of reading + 11 mV	
	(50 to 100) kHz	0.23 % of reading + 45 mV	


## Electrical – DC/Low Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
DC Resistance – Source <sup>2</sup> (Fixed-Simulated Values)	1 $\Omega$	98 $\mu\Omega/\Omega$	Comparison to Fluke 5720A Multiproduct Calibrator
	1.9 $\Omega$	96 $\mu\Omega/\Omega$	
	10 $\Omega$	24 $\mu\Omega/\Omega$	
	19 $\Omega$	25 $\mu\Omega/\Omega$	
	100 $\Omega$	11 $\mu\Omega/\Omega$	
	190 $\Omega$	11 $\mu\Omega/\Omega$	
	1 k $\Omega$	9.4 m $\Omega/k\Omega$	
	1.9 k $\Omega$	10 m $\Omega/k\Omega$	
	10 k $\Omega$	10 m $\Omega/k\Omega$	
	19 k $\Omega$	10 m $\Omega/k\Omega$	
	100 k $\Omega$	12.6 m $\Omega/k\Omega$	
	190 k $\Omega$	29.5 m $\Omega/k\Omega$	
	1 M $\Omega$	22 $\Omega/M\Omega$	
	1.9 M $\Omega$	125 $\Omega/M\Omega$	
	10 M $\Omega$	74 $\Omega/M\Omega$	
	19 M $\Omega$	0.65 k $\Omega/M\Omega$	
	100 M $\Omega$	0.6 k $\Omega/M\Omega$	

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ( $k=2$ ), corresponding to a confidence level of approximately 95%.

### Notes:

1. Based on an accredited calibration by the manufacturer, used at the temperature in which the Multiproduct Calibrator was calibrated ( $t_{cal} = \pm 5^\circ\text{C}$ ) and assuming the instrument is zeroed at least every seven days or when the ambient temperature changes more than  $5^\circ\text{C}$ .
2. Unless otherwise specified in the far-right column, the calibration procedure or method was written internally.
3. The legal entity for this Multisite location is Transcat, Inc.

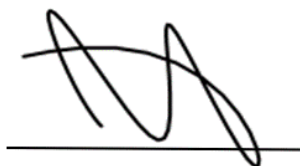

Jason Stine, Vice President